

Elevate the everyday

enVista
HYDROPHOBIC ACRYLIC IOL ASPIRE™

enVista
HYDROPHOBIC ACRYLIC IOL ASPIRE™ TORIC

Intermediate
Optimized
monofocal IOLs



BAUSCH + LOMB

enVista
ASPIRE™



Elevate the everyday

Transcend the boundaries of standard monofocals and deliver your patients an IOL designed for the modern world — a fusion of uncompromised distance vision with an optic designed for a broader depth of focus.

Built on innovative, Intermediate Optimized (IO) optics and harmonized with Controlled Curvature Change (3C) technology, enVista Aspire™ is a right option for your patients as they **navigate their increasingly tech-infused lifestyles.**



A monofocal IOL for the modern world

Patients are navigating their world with more complexities than ever before. As the world progresses, so should their standard of cataract care. The need for broader range of vision is apparent, as adults spend more than 13 hours a day interacting with digital devices.¹ As a surgeon, enVista Aspire™ provides you with the opportunity to deliver modern expectations.

- Novel optics built on a proven platform that is trusted around the world with more than 8 million implantations²
- In optical bench testing, enVista Aspire™ demonstrated a broader depth of focus compared to enVista™ AO (Advanced Optics) monofocal IOLs³
- The original glistening-free optic material



1. UnitedHealthcare. UnitedHealthcare Screen Time Report 2020. Published 2020. Accessed October 17, 2023. Available at: <https://www.uhc.com/content/dam/uhcdotcom/en/BrokersAndConsultants/UnitedHealthcare-Screen-Time-Report-2020.pdf>
2. enVista® and Enhanced enVista® shipments extract 2011-June 2024
3. enVista Aspire™ Instructions for use, Figure 2.

Outstanding performance and optical engineering are built into the design of every enVista™ lens


Central zone

enVista Aspire™'s Intermediate Optimized (IO) central zone utilizes higher-order aspheric coefficients on the posterior surface to create a broader depth of focus.

Featuring 3C (Controlled Curvature Change) technology, enVista Aspire™ optics are designed to harmonize the geometric power profile outward between the central base power and power at the periphery.

enVista Aspire™ demonstrated 1.25 D of continuous depth of focus⁴

enVista Aspire™ IOL Power Surface Plot showing the power distribution on the posterior side of the Aspire IOL optic.

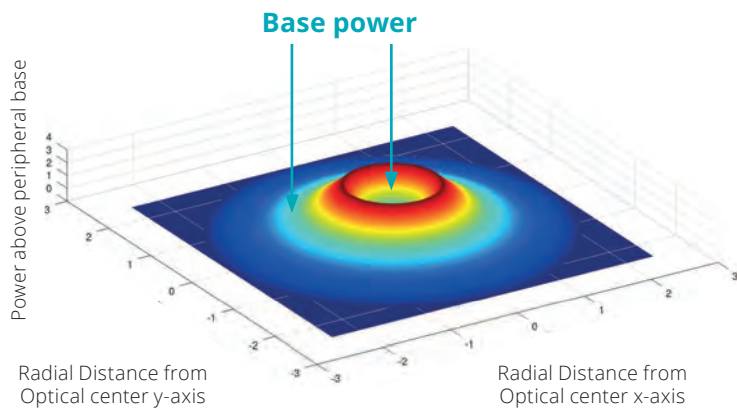

This image is not a topographical map of the lens, it is a power map of the lens


Optic power profile

The unique optic of enVista Aspire™ creates a gradual transitional distribution of light energy from centre to the periphery.

4. BAUSCH+LOMB data on file: Aspire Optical Characterization Rev A - December 2022.

5. Juan Antonio Azor, Fidel Vega, Jesús Armengol, María S. Millán. Characterization of various presbyopia-correcting intraocular lenses on optical bench. Comparative study. Grupo de Óptica Aplicada y Procesado de Imagen (GOAPI). Department of Optics and Optometry Universitat Politècnica de Catalunya BARCELONATECH


6. Feltrin de Barros et al, "Optical Performance and Refractive Outcomes of a New Monofocal Intraocular Lens With Intermediate Optimized Optics", J Ref Surg; 41(10): e1069-e1075 (2025)

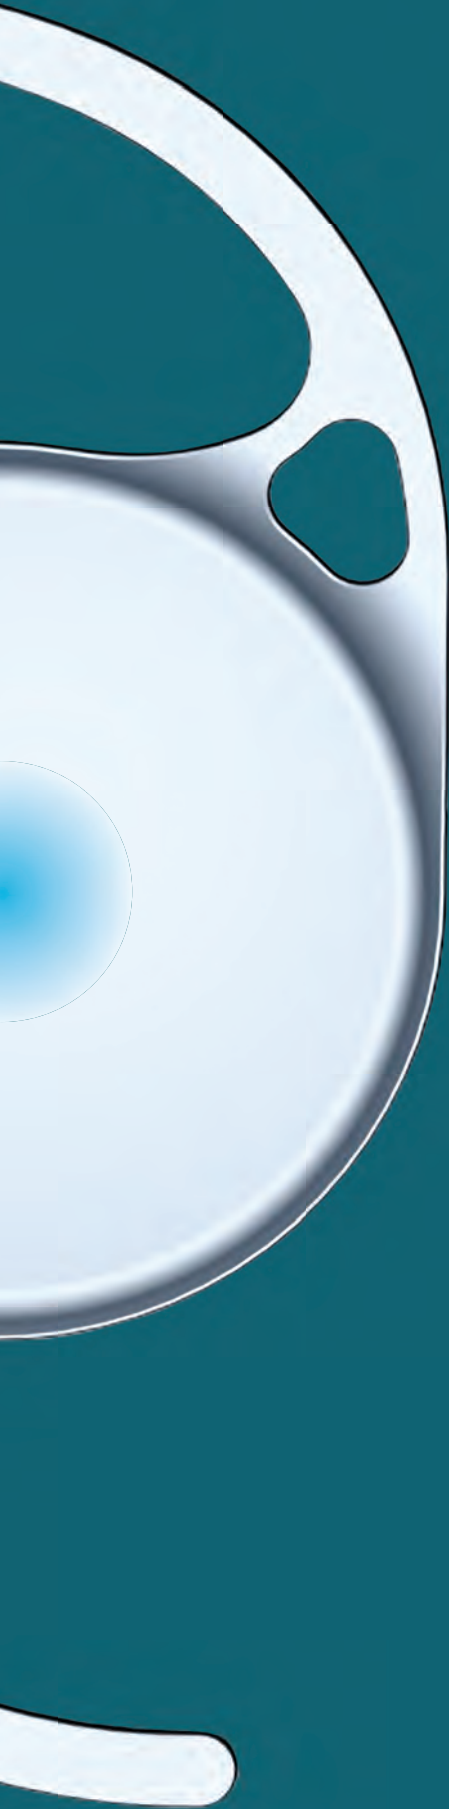

Uncompromising distance vision

Optical bench testing for enVista Aspire™ (Intermediate Optimized Optic) showed an Expected Visual Acuity (EVA) of 6/4.8 for distance vision⁵

enVista Aspire™ Expected Visual Acuity (EVA) at 3.00 mm pupil size, +0.27 μm corneal spherical aberration and 550 nm monochromatic light.

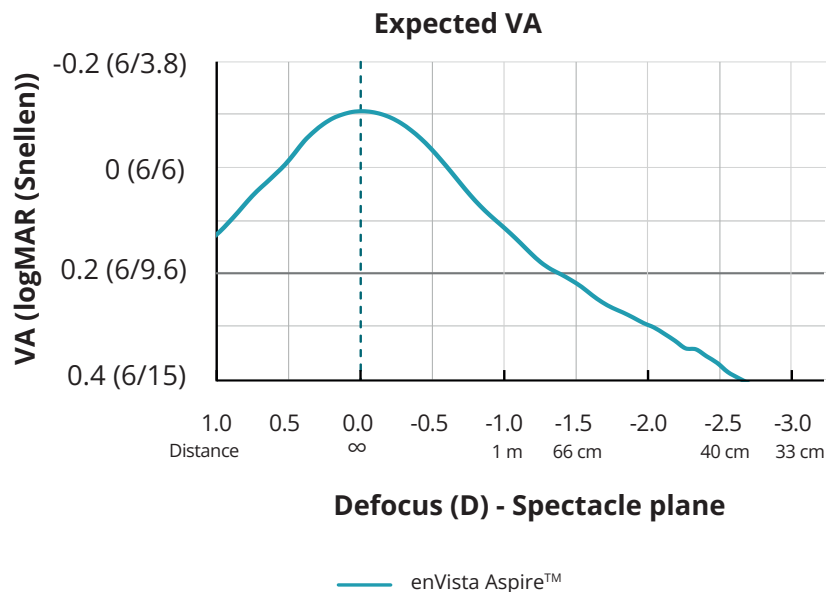


Clinical Results

A prospective observational study in 2025 demonstrated excellent monocular distance vision (mean UDVA 6/6.7), useful intermediate (mean DCIVA 6/10) and functional near vision (mean DCNVA 6/11.4)⁶

Intermediate Optimized optic

Expected Visual Acuity at 3.00 mm pupil size, +0.27 μm corneal spherical aberration and 550 μm monochromatic light.

In optical bench testing, enVista Aspire™ demonstrated similar depth of focus compared to TECNIS Eyhance™⁷

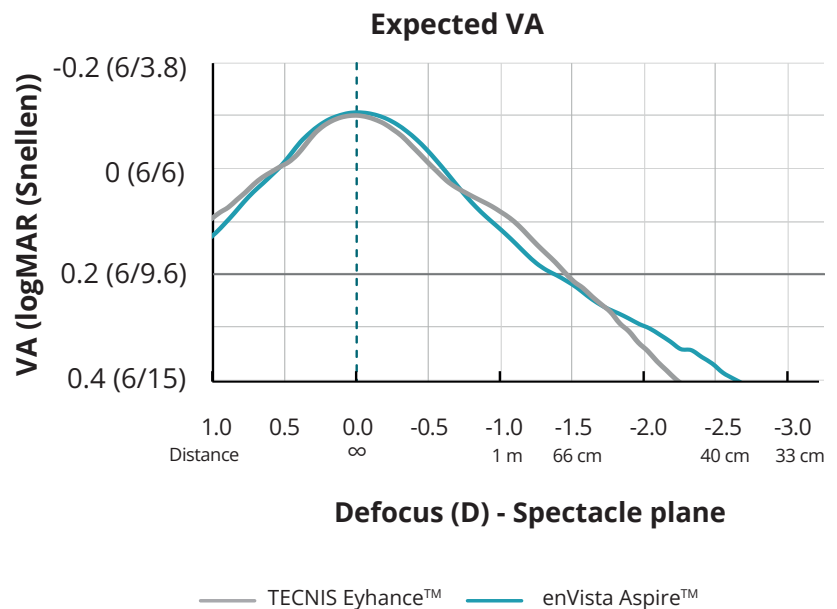

This expected Visual Acuity (EVA) is a pre-clinical metric, estimated using a formula from the through focus MTFa obtained with the 3.00 mm pupil size.^{8,9}

This MTFa results from the integration of MTF function in a range of spatial frequencies and has been shown to strongly correlate with average clinical visual acuity.^{9,10}

The EVA provides a useful tool to predict the expected visual performance of a lens.

7. Juan Antonio Azor, Fidel Vega, Jesus Armengol, Maria S. Millan. Characterization of various presbyopia-correcting intraocular lenses on optical bench. Comparative study. Grupo de Optica Aplicada y Procesado de Imagen (GOAPI). Department of Optics and Optometry Universitat Politècnica de Catalunya BARCELONATECH

8. Alarcon A, Canovas C, Rosen R, et al. Preclinical metrics to predict through-focus visual acuity for pseudophakic patients. Biomed Opt Express. 2016;7(5):1877-1888

9. American National Standards Institute (ANSI) Z80.35-2018, "Extended depth of focus intraocular lenses"

10. Vega F., Met al "Visual acuity of pseudophakic patients predicted from in-vitro measurements of intraocular lenses with different design," Biomed. Opt. Express 9(10),4893-4906 (2018)

Monofocal for the modern world





In optical bench testing enVista Aspire™ is less sensitive to tilt and decentration when compared with TECNIS Eyhance™



Decentration is much more frequent than one might think


A large series of 395 eyes reported an average IOL decentration after uncomplicated cataract surgery of 0.40 ± 0.2 mm (range 0 to 1.7 mm)¹¹

Comparative MTF for tilt and decentration at 3.00 mm pupil size and +0.27 μ m corneal spherical aberration⁷

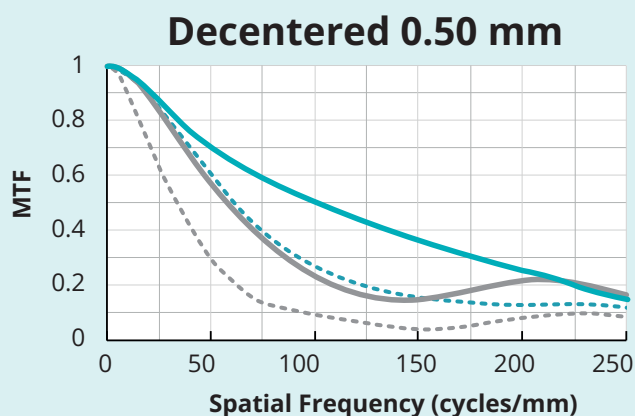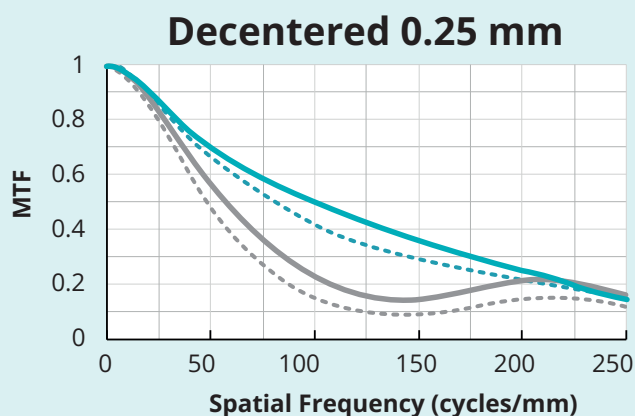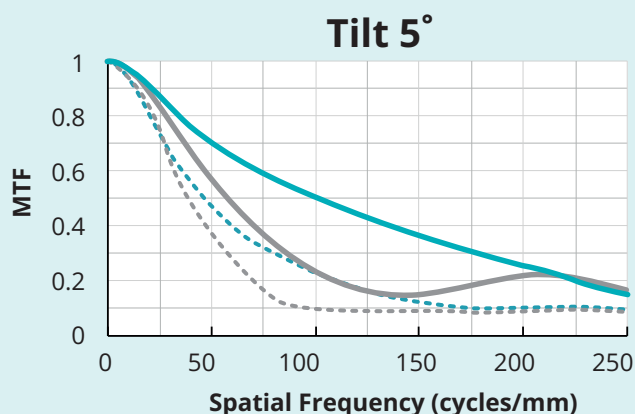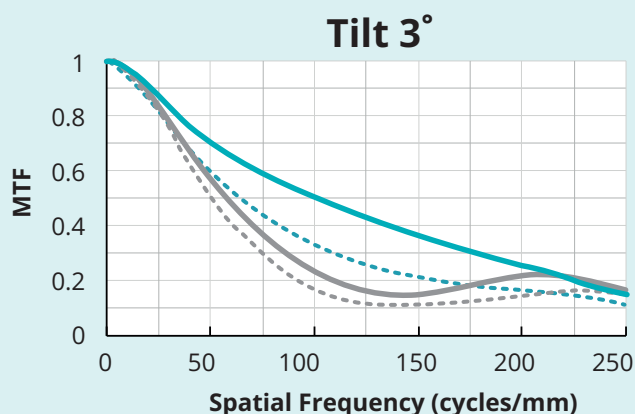


— enVista Aspire™ - - - enVista Aspire™ tilted or decentered — TECNIS Eyhance™ - - - TECNIS Eyhance™ tilted or decentered

Correcting astigmatism with MORE precision*

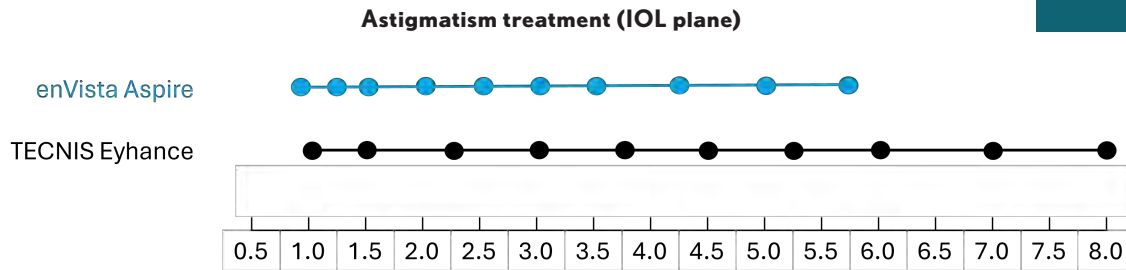



* Compared to range of cylinders offered with Tecnis Eyhance Toric, as listed on the Prescribed List in November 2025

Thanks to our extended range of cyls and ultra low +0.90 D, enVista Aspire™ Toric covers 68 % of the cataract surgery population with > +0.50 D of corneal astigmatism^{12*}

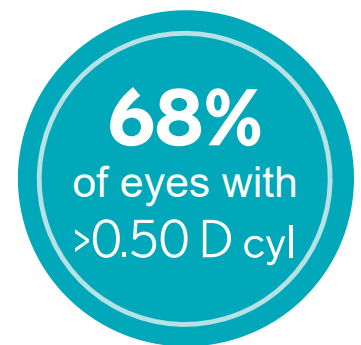

A small amount of astigmatism (as little as 0.50 D) has the potential to affect functional and low contrast visual acuity¹³ and has an impact on the visual comfort of computer users.¹³

With more cylinder powers at the lower end of astigmatism correction, greater precision can be achieved where it matters the most.

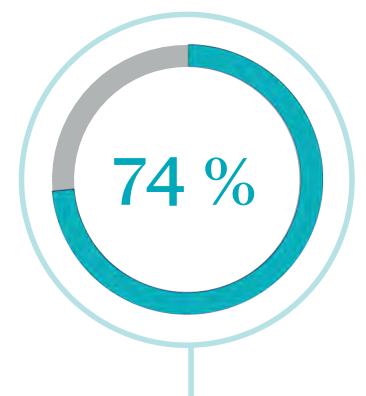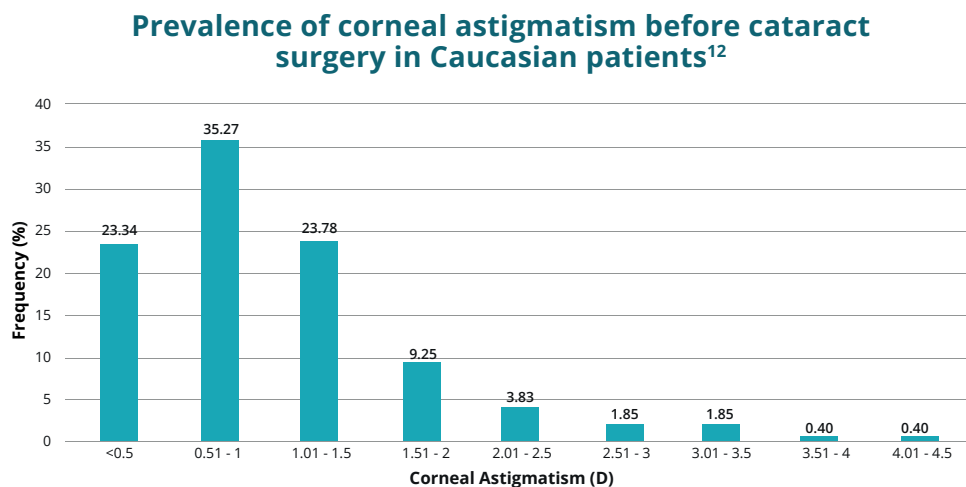

of cataract patients have less than 1.25 D of corneal astigmatism¹⁴

Corneal astigmatism distribution in 0.50 D steps in the entire sample (757 eyes).

* Calculation from the Bernardo histogram Figure 1. Assuming a Linear interpolation of the area under the curve of the range of cylinders.

12. De Bernardo M, Zeppa L, Cennamo M, Iaccarino S, Zeppa L, Rosa N. Prevalence of Corneal Astigmatism before Cataract Surgery in Caucasian Patients. European Journal of Ophthalmology. 2014;24(4):494-500. doi:10.5301/ejo.5000415

13. Miller AD, Kris MJ, Griffiths AC. Effect of small focal errors on vision. Optom Vis Sci. 1997;74(7):521-526. Novis C. Astigmatism and Toric Intraocular Lenses. Current Opinion in Ophthalmology 2000; Vol. 11, Issue 1: 47-50.


14. Holland E J. Treating Astigmatism With Torics. In: Cataract & Refractive Surgery Today Supplement. 2010 Feb. p. 5-6. Available from: https://crstoday.com/wpcontent/themes/crst/assets/downloads/0210_supp.pdf

Lock in rotational stability you can count on




Accuset™ Haptics - designed for refractive predictability and stable centration¹⁴⁻¹⁶


- **Fenestrated haptics** to reduce stress transferring from the haptic to the optic
- **Haptics designed to** maximize the contact angle against the capsular bag

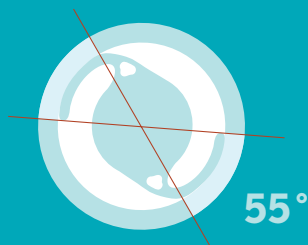

enVista™ IOL¹⁷
(Based on 10 mm capsular bag)



AcrySof IQ®¹⁸
(Based on 10 mm capsular bag)

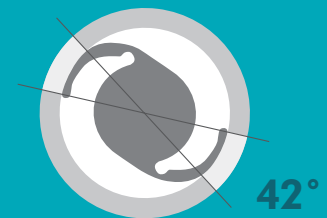

Tecnis IOL®¹⁹
(Based on 10 mm capsular bag)



100% of eyes ≤ 5° rotation

enVista™ Toric delivered proven rotational stability **from visit 1-2 months to visit 4-6 months²⁰**

14. Parker et al. Safety and effectiveness of a glistening-free single-piece hydrophobic acrylic intraocular lens (enVista). Clin Ophthalmol. 2013;7: 1905-1912.
 15. P. Heiner et al. Safety and effectiveness of a single-piece hydrophobic acrylic intraocular lens (enVista®) – results of a European and Asian-Pacific study. Clin Ophthalmol. 2014;8: 629-635.
 16. Garzon et al. Evaluation of Visual Outcomes After Implantation of Monofocal and Multifocal Toric Intraocular Lenses. J Refract Surg. 2015;31(2):90-97.
 17. BAUSCH + LOMB data on file : Intraocular lens design verification report- July 2016.
 18. BAUSCH + LOMB data on file: IOL competitive benchmarking study report_DEC 2009.
 19. PMA P980040/S039: FDA Summary of Safety and Effectiveness Data_Tecnis Toric IOL.
 20. enVista Toric data (MX60T). Packer M, Williams JJ, Feinerman G, Hope RS. Prospective multicenter clinical trial to evaluate the safety and effectiveness of a new glistening-free one-piece acrylic toric intraocular lens. Clinical Ophthalmology 2018;12: 1031-1039

The enVista™ Toric Calculator

Your partner in accuracy

The enVista™ Toric calculator integrates the Emmetropia Verifying Optical (EVO) Toric Formula, an advanced IOL formula for cataract surgery.²¹

It is based on the theory of emmetropization and generates an 'emmetropia factor' for each eye. As a thick lens formula, it takes into account of the optical dimensions of the eye, and can handle different IOL geometry and powers.


When calculating toric IOLs, it combines:

Theoretical posterior cornea astigmatism prediction


Thick lens modelling

Dynamically interconnected prediction of IOL power and toricity

A retrospective evaluation of EVO Toric Formula performed in a multi-centered clinical trial including 10 surgeons, based on 109 eyes implanted with enVista™ toric²² showed:



Residual
astigmatism
prediction error



Calculator predicted orientation
matched the theoretical post-
operative refractive astigmatism



Arithmetic mean
residual astigmatism
prediction error

The Barrett Toric Calculator and EVO Toric Calculator had similar performance with regards to their astigmatism prediction accuracy.



Scan to access
the EVO toric calculator
<https://www.evoiolcalculator.com>


21. <https://evoiolcalculator.com/start.aspx>

22. Pantanelli SM, Sun A, Kansara N, Smits G. Comparison of Barrett and Emmetropia Verifying Optical Toric Calculators. Clin Ophthalmol. 2022;16:177-182 <https://doi.org/10.2147/OPHTH.S346925>

enVista ASPIRE™

HYDROPHOBIC ACRYLIC IOL

SKU EAxxxx

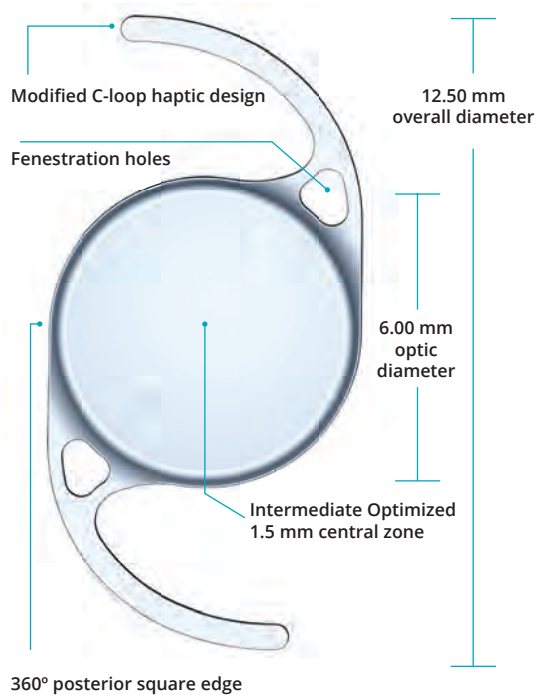

MATERIAL

- Hydrophobic acrylic glistening-free
- UV filter (10 % cut-off wavelength: 389 nm)
- Refractive index: 1.53 at 35°C

DESIGN

- Intermediate Optimized Toric IOL with posterior high order aspheric surface
- One piece, biconvex
- Modified C-loop haptic design
- 360° posterior square edge
- Haptic with fenestration holes
- Optic diameter: 6.00 mm
- Overall diameter: 12.50 mm

DIOPTER RANGE

enVista Aspire™

From +6.00 D to +34.00 D (0.50 D steps)

enVista Aspire™ TORIC

Spherical equivalent power:

From +6.00 D to +34.00 D (0.50 D steps)


Cylinder power – IOL Plane: 0.90 D / +1.25 D / +1.50 D / +2.00 D / +2.50 D / +3.00 D / +3.50 D / +4.25 D / +5.00 D / +5.75 D

Cylinder power - Corneal plane: +0.64 D / +0.90 D / +1.06 D / +1.40 D / +1.76 D / +2.11 D / +2.45 D / +2.98 D / +3.50 D / +4.03 D

enVista ASPIRE™ TORIC

HYDROPHOBIC ACRYLIC IOL

SKU ETAxxx+xxx

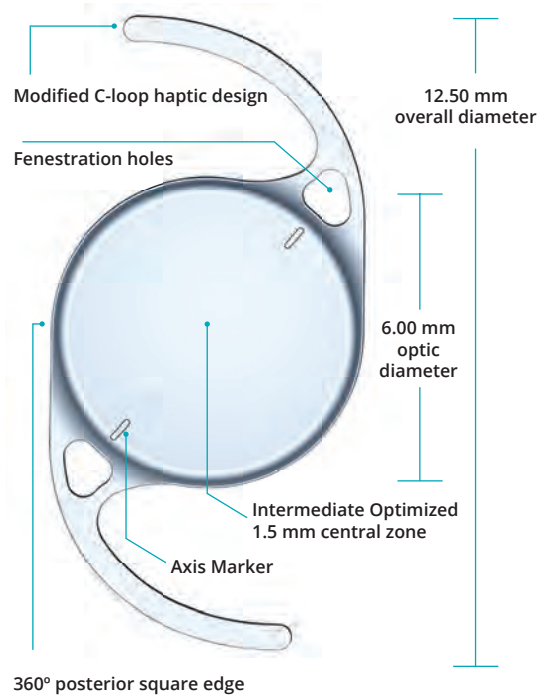

DELIVERY SYSTEM

Non-preloaded

BLIS (screw type, controlled delivery) reusable inserter and single use cartridge

Inserter: BLIS-R1 (1 Unit/box)

Cartridge: BLIS-X1 (10 Units/box)

Recommended incision size ≥ 2.2 mm



CONSTANTS*

OPTIC CONSTANT

SRK/T Constant A: 119.1

Hoffer Q / Holladay 2 ACD: 5.61

Holladay 1 Surgeon Factor: 1.85

Haigis: a0: 1.46 / a1: 0.40 / a2: 0.10

Barrett Lens Factor: 1.94

Barrett Design Factor: <blank>

ULTRASONIC CONSTANT

Constant A: 118.7

ACD: 5.37

Surgeon factor: 1.62

* Constants are estimates only. It is recommended that each surgeon develops their own values.



enVista
HYDROPHOBIC ACRYLIC IOL
ASPIRE™

enVista
HYDROPHOBIC ACRYLIC IOL
ASPIRE™ TORIC

Transcend the boundaries of standard monofocals and deliver your patients an IOL designed for the modern world.

 @BauschSurgical

 Bausch + Lomb Surgical

www.bauschsurgical.com*

* International website

© 2025 Bausch + Lomb Incorporated. All rights reserved.

®/™ are trademarks of Bausch & Lomb Incorporated or its affiliates. All other brand/product names are trademarks of the respective owners.

Bausch & Lomb (Australia) Pty Ltd. ABN 88 000 222 408. Level 2, 12 Help Street, Chatswood NSW 2067 Australia. (Ph 1800 251 150)

New Zealand Distributor: Toomac Ophthalmic. 32D Poland Road, Glenfield 0627 Auckland New Zealand (Ph 0508 443 5347)

enVista_ASPIRE_HCP_Brochure_EASP.0002.AU.25

BAUSCH + LOMB

CATARACT
GLAUCOMA
REFRACTIVE
RETINA
VISUALIZATION